


surgical spirit pro

George & Jenny

Spectrum Peak Pick Report

07/02/2017 17:24:12

Data Set: BEN_1.0_90M_172256.spc - RawData

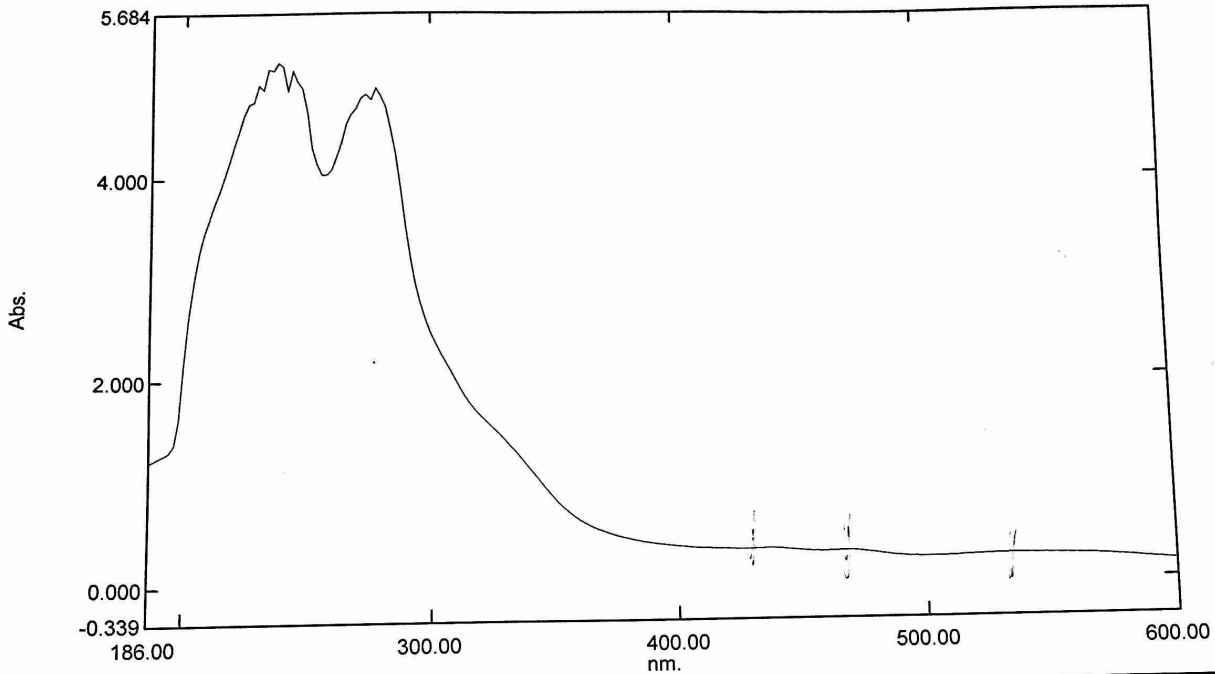

[Measurement Properties]
 Wavelength Range (nm.): 185.00 to 600.00
 Scan Speed: Medium
 Sampling Interval: 2.0
 Auto Sampling Interval: Disabled
 Scan Mode: Auto

[Instrument Properties]
 Instrument Type: UV-2600 Series
 Measuring Mode: Absorbance
 Slit Width: 5.0
 Accumulation time: 0.1 sec.
 Light Source Change Wavelength: 370.0 nm
 Detector Unit: Direct
 S/R Exchange: Normal
 Stair Correction: OFF

[Attachment Properties]
 Attachment: None

[Operation]
 Threshold: 0.0010000
 Points: 4
 InterPolate: Disabled
 Average: Disabled
 Data Process: Point Pick
 Template: Holmium.spt

[Sample Preparation Properties]
 Weight:
 Volume:
 Dilution:

No.	P/V	Wavelength	Abs.	Description
1	⊕	536.00	0.247	
2	⊕	468.00	0.296	
3	⊕	436.00	0.327	
4	⊕	278.00	4.914	
5	⊕	238.00	5.182	
6	⊖	502.00	0.227	
7	⊖	458.00	0.292	
8	⊖	428.00	0.321	
9	⊖	256.00	4.039	

GRAPES